



Aalborg Universitet

AALBORG UNIVERSITY
DENMARK

Hemoglobin variants found in relation to HbA1c testing

high occurrence of Hb Athens-Georgia in the Northern Jutland, Denmark

Nybo, Jan; Hansen, Anette Tarp; Petersen, Jesper Brix; Brock, Axel

Published in:
Clinical Chemistry and Laboratory Medicine

DOI (link to publication from Publisher):
[10.1515/cclm-2018-0902](https://doi.org/10.1515/cclm-2018-0902)

Publication date:
2019

Document Version
Publisher's PDF, also known as Version of record

[Link to publication from Aalborg University](#)

Citation for published version (APA):

Nybo, J., Hansen, A. T., Petersen, J. B., & Brock, A. (2019). Hemoglobin variants found in relation to HbA1c testing: high occurrence of Hb Athens-Georgia in the Northern Jutland, Denmark. *Clinical Chemistry and Laboratory Medicine*, 57(6), E108-E110. <https://doi.org/10.1515/cclm-2018-0902>

General rights

Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the public portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the public portal -

Take down policy

If you believe that this document breaches copyright please contact us at vbn@aub.aau.dk providing details, and we will remove access to the work immediately and investigate your claim.

Letter to the Editor

Jan Nybo*, Anette Tarp Hansen, Jesper Brix Petersen and Axel Brock

Hemoglobin variants found in relation to HbA_{1c} testing: high occurrence of Hb Athens-Georgia in the Northern Jutland, Denmark

<https://doi.org/10.1515/cclm-2018-0902>

Received June 14, 2018; accepted September 10, 2018; previously published online October 8, 2018

Keywords: capillary; electrophoresis; glycated hemoglobin A; Hb Athens-Georgia; hemoglobinopathies.

To the Editor,

Hemoglobinopathies are usually divided into those caused by an impaired synthesis of one or more hemoglobin chains (α -, β - and γ -thalassemia) and those caused by inherited structural alteration of one of the globin chains (hemoglobin variants). Heterozygotes of a mutation related to the hemoglobin synthesis in most cases will be asymptomatic, whereas homozygosity – especially for α -thalassemia, β -thalassemia, and certain hemoglobin variants – will result in serious clinical conditions. Mutations related to the hemoglobin synthesis are very common. Some mutations are endemic in certain geographic regions (i.e. Hb E and α -thalassemia in the South-eastern Asia, Hb S and Hb C in Central and Western Africa, and β -thalassemia in the Eastern Mediterranean countries), whereas the more uncommon mutations are found all over the world [1]. More than 450 mutations causing α - or β -thalassemia and more than 1300 mutations causing hemoglobin variants have so far been reported in the Database of Human Hemoglobin Variants and Thalassemias [2]. Probably, around 270 million people carry variant β -globin genes [1]. Nevertheless, hemoglobinopathies have been considered rare in Caucasians.

Depending on the method used for HbA_{1c} testing, the presence of a hemoglobin variant may cause analytical

interference [3–5] leading to a misinterpretation of the diabetes status of the patient concerned. Moreover, hemoglobin variants cause an increased erythrocyte turn over which by itself will result in a low HbA_{1c} value [5]. Capillary electrophoresis provides a good separation of the different hemoglobin fractions in normal blood samples [6]. It also provides a good separation in blood samples from individuals being heterozygous for HbS, HbC, HbD and HbE, with analytically valid HbA_{1c} results as a consequence [4]. Furthermore, capillary electrophoresis enables the detection of a great number of other hemoglobinopathies, including persistent HbF [7].

During an 18-month period (February 2016–July 2017) 139,000 individuals in Northern Jutland, Denmark, were routine tested by capillary electrophoresis using a Capillary 3 Tera and the CAPI 3 HbA_{1c} kit (Sebia, France) according to the protocol provided by the manufacturer. Curves with a profile indicating the presence of a hemoglobin variant were registered in 163 of the 139,000 tested individuals of these, a complementary test for hemoglobinopathy was performed in 91 randomly selected cases (56% corresponding to a background population of 77,600). The procedure for detecting hemoglobinopathy included fractionation by ultra-performance liquid chromatography on a Waters Acquity ultra-performance liquid chromatography system (Waters Corporation, Milford, MA, USA) using a PolyCAT A column (3 μ m, 1500 Å) (PolyLC Inc., Columbia, MD, USA). When either fractionation (HbA_{1c} or UPLC) was suspect for a variant hemoglobin, sequencing of the β (HBB) and/or α globin genes (*HBA1* and *HBA2*) were performed on a 3500 Genetic Analyzer (Applied Biosystems, Foster City, CA, USA) using BigDye v. 3.1 sequencing chemistry (Applied Biosystems). Table 1 shows the results obtained.

In total, we identified 22 different hemoglobin variants, including persistent Hb F and Hb H disease. Only 33 of the 91 individuals carried the variants Hb E, Hb S, or Hb C. In the remaining 58 cases, we identified 19 different hemoglobin variants. Thirty-three of these, all with Danish names, carried the globally uncommon variant

*Corresponding author: Jan Nybo, MD, Department of Clinical Biochemistry, Aalborg University Hospital, Aalborg, Denmark, Phone: +45 23 99 41 12, E-mail: j.nybo@rn.dk

Anette Tarp Hansen and Axel Brock: Department of Clinical Biochemistry, Aalborg University Hospital, Aalborg, Denmark

Jesper Brix Petersen: Department of Hematology, Copenhagen University Hospital, Herlev, Denmark

Table 1: Hemoglobin variants accidentally found in relation to routine HbA_{1c} testing.

α Chain cluster	
Hb H (α thalassemia, deletion)	2
Unnamed (Thr 67 Ile; HBA1:c.203C>T)	1
Unnamed (Val 93 Leu; HBA1:c.280G>T)	1
Hb Cibeles (Gly 25 Asp; HBA2:c.77G>A)	1
Hb St. Tuiden (Asn 68 His; HBA2:c.205A>C)	1
β Chain cluster	
Hb Lepore (Δ-β thalassemia, deletion)	1
Hb F (HPFH; deletion)	2
Hb Doha (Val 1 Glu; HBB:c.5T>A)	1
Hb C (Glu 6 Lys; HBB:c.19G>A)	3
Hb S (Glu 6 Val; HBB:c.20A>T)	8
Hb J-Lens (Ala 13 Asp; HBB:c.41C>A)	1
Hb E (Glu 26 Lys; HBB:c.79G>A)	22
Hb Tacoma (Arg 30 Ser; HBB:c.93G>T)	1
Hb Athens-GA (Arg 40 Lys; HBB:c.122G>A)	33
Hb Niteroi (del CD43/45; HBB:c.130_138delGAGTCCTTT)	1
Hb Aalborg (Gly 74 Arg; HBB:c.223G>C)	2
Hb J-Iran (His 77 Asp; HBB:c.232C>G)	1
Hb Helsinki (Lys 82 Met; HBB:c.248A>T)	2
Hb Köln (Val 98 Met; HBB:c.295G>A)	1
Unnamed (Leu 105 Val; HBB:c.316C>G)	1
Hb Villejuif (Tyr 123 Ile; HBB:c.371C>T)	3
Hb Hope (Gly 136 Asp; HBB:c.410G>A)	2
Total	91

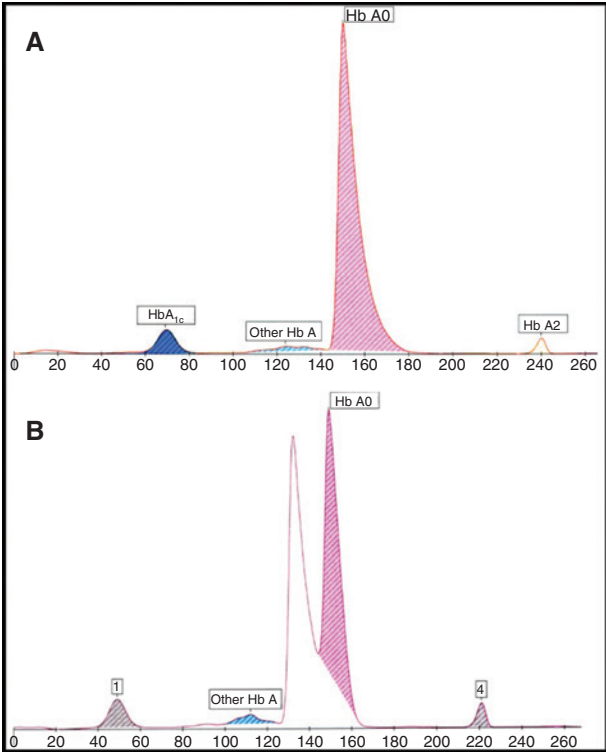


Figure 1: Electropherograms from the Capillarys 3 automated multicapillary zone electrophoresis system. Normal HbA_{1c} electropherogram (A), and a HbA_{1c} electropherogram from a patient with the Hb variant, Hb Athens-Georgia (B).

Hb Athens-Georgia (Figure 1). Three of the detected variants (α1-chain: Thr 67 Ile, Val 93 Leu; β-chain: Leu 105 Val) were not registered in the Database of Human Hemoglobin Variants and Thalassemias [2].

Hb Athens-Georgia is considered a rare variant found in a few Caucasian families in the south-eastern USA and Belgium [2, 8], but in 1988 the variant was also found in a Danish family [9]. Hb Athens-Georgia is not detected by cation-exchange high-performance liquid chromatography, nor by boronate affinity chromatography, which are commonly used techniques for measuring HbA_{1c} [8]. The variant is clinically silent [2]. The high occurrence of Hb Athens-Georgia in Northern Jutland, corresponding to an estimated prevalence of 43:100,000 (equivalent to 33/77,600), is unexplained. The high occurrence may be due to a local founder effect or to a general underreporting due to the asymptomatic phenotype and the widespread use of cation-exchange high-performance liquid chromatography or boronate affinity chromatography for HbA_{1c} testing. The occurrence of Hb Athens-Georgia in other parts of Denmark is unknown.

Our findings confirm that the prevalence of clinically silent Hb-variants may be higher than expected so far [10]. HbA_{1c} is defined as the fraction of HbA carrying a covalently bound glucose molecule to the N-terminal valine of the β-chains. Depending on the method used, some of the hemoglobin variants do not interfere with the actual measurement of HbA_{1c} [4, 7], but some of them will, i.e. due to an increased erythrocyte turn over, interfere with the interpretation of the result obtained.

Author contributions: All the authors have accepted responsibility for the entire content of this submitted manuscript and approved submission.

Research funding: None declared.

Employment or leadership: None declared.

Honorarium: None declared.

Competing interests: The funding organization(s) played no role in the study design; in the collection, analysis, and interpretation of data; in the writing of the report; or in the decision to submit the report for publication.

References

1. Birgens H, Ljung R. The thalassaemia syndromes. Scand J Clin Lab Invest 2007;67:11–26.
2. HbVar: A Database of Human Hemoglobin Variants and Thalassemias. Available at: <http://globin.bx.psu.edu/cgi-bin/hbvar/couner>. Accessed: 8 Jan 2018.

3. Little RR, La'ulu SL, Hanson SE, Rohlfing CL, Schmidt RL. Effects of 49 different rare Hb variants on HbA_{1c} measurement in eight methods. *J Diabetes Sci Technol* 2015;9:849–56.
4. Rohlfing C, Hanson S, Weykamp C, Siebelder C, Higgins T, Molinaro R, et al. Effects of hemoglobin C, D, E and S traits on measurements of hemoglobin A_{1c} by twelve methods. *Clin Chim Acta* 2016;455:80–3.
5. Rhea JM, Molinaro R. Pathology Consultation on HbA_{1c} methods and interferences. *Am J Clin Pathol* 2014;141:5–16.
6. Jaisson S, Leroy N, Meurice J, Guillard E, Gillery P. First evaluation of Capillarys 2 Flex Piercing® (Sebia) as a new analyzer for HbA_{1c} assay by capillary electrophoresis. *Clin Chem Lab Med* 2012;50:1769–75.
7. van Zwieten R, Veldthuis M, Delzenne B, Berghuis J, Groen J, Ait Ichou F, et al. Hemoglobin analyses in the Netherlands reveal more than 80 different variants including six novel ones. *Hemoglobin* 2014;38:1–7.
8. Peeters B, Brandt I, Desmet K, Harteveld CL, Kieffer D. Hb Melusine and Hb Athens-Georgia: potentially underreported in the Belgian population? Four cases demonstrating the lack of detection using common CE-HPLC methods either for glycated hemoglobin HbA_{1c} analysis or Hb variant screening. *Acta Clin Belg* 2016;71:458–61.
9. Blanke S, Johnsen A, Wimberley PD. HB Athens-Georgia [β 40(C6)ARG→LYS] in a Danish family. *Hemoglobin* 1989;13:181–3.
10. Strickland SW, Campbell ST, Little RR, Bruns DE, Bazydlo LA. Prevalence of rare hemoglobin variants identified during measurements of HbA_{1c} by capillary electrophoresis. *Clin Chem* 2017;63:1901–2.